

Chap. 6 Proportional Counters

Consider the drift motion of an ion in a simple ion chamber. The ions will have a thermal velocity plus a component along the field lines. Then after traveling for a mean-free-path they will undergo a collision that will randomize their velocity and they start over. What if the energy gain in one step is greater than the FIP of the buffer gas?

$$\Delta E \sim q_e \varepsilon \Delta x \quad \text{where} \quad \Delta x \sim \lambda_{MFP} \quad \rightarrow \quad q_e \varepsilon \sim \frac{\Delta E}{\lambda_{MFP}}$$


$$\lambda_{MFP} = \frac{1}{\sqrt{2} \pi d^2 \rho_n} \quad (\text{for molecules})$$

$$\lambda_{MFP}(\text{air}) = 6.6 \text{ mm} / \text{Pa} \quad \text{or} \quad 6 \times 10^{-8} \text{ m at } 1 \text{ atm}$$

$$q_e \varepsilon \sim \frac{FIP}{6 \times 10^{-8} \text{ m}} \sim 200 \text{ MV} / \text{m}$$

This value is too large for a nominal detector and so no multiplication of/by molecular ions.



However, MV/m = keV/mm is achievable. Recall that the electrons will have much longer mean-free paths – electrons can be multiplied or “avalanched”.

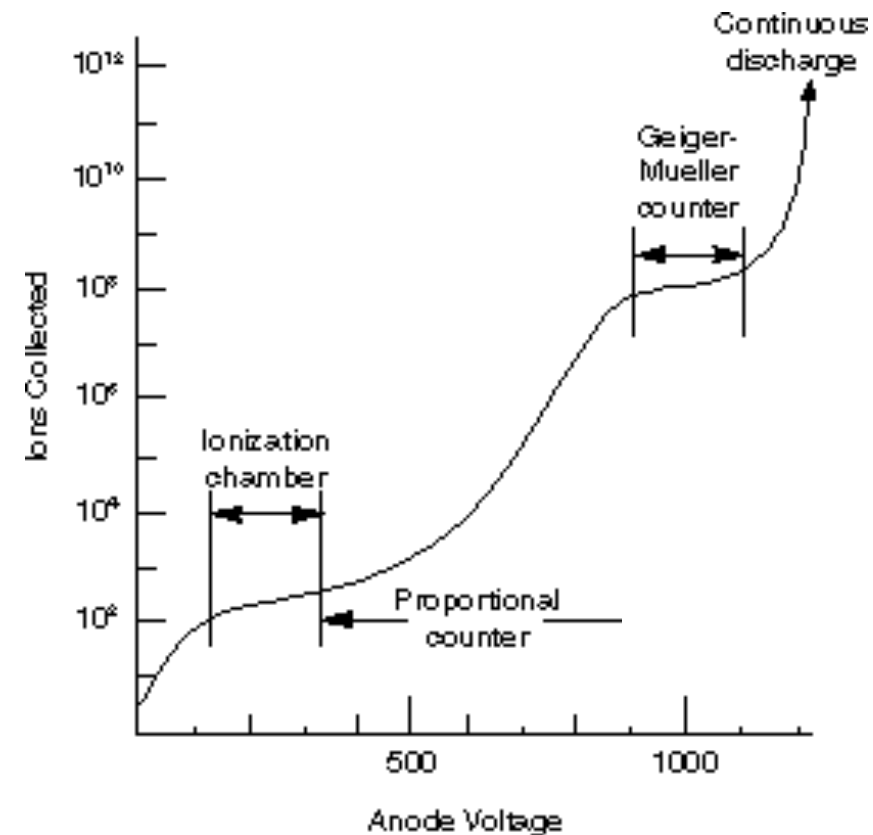

Similar to qualitative Fig. 6.2 Knoll, 3rd Ed.

Proportional Counters – Multiplication on Wires

Proportional counters are gas filled and generally use wire anodes (recent devices use thin lines on printed circuit boards).

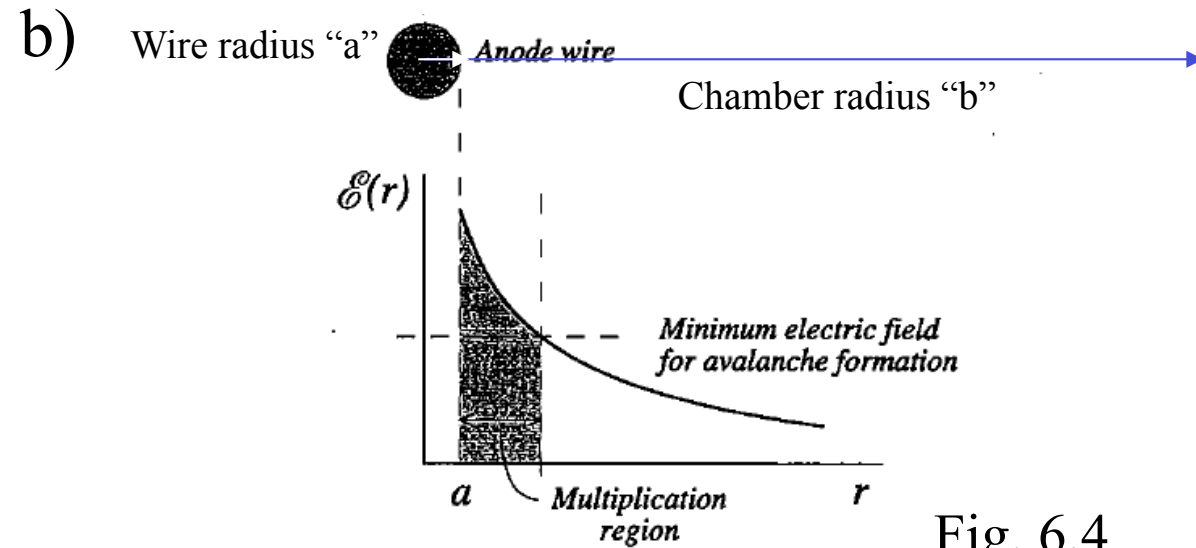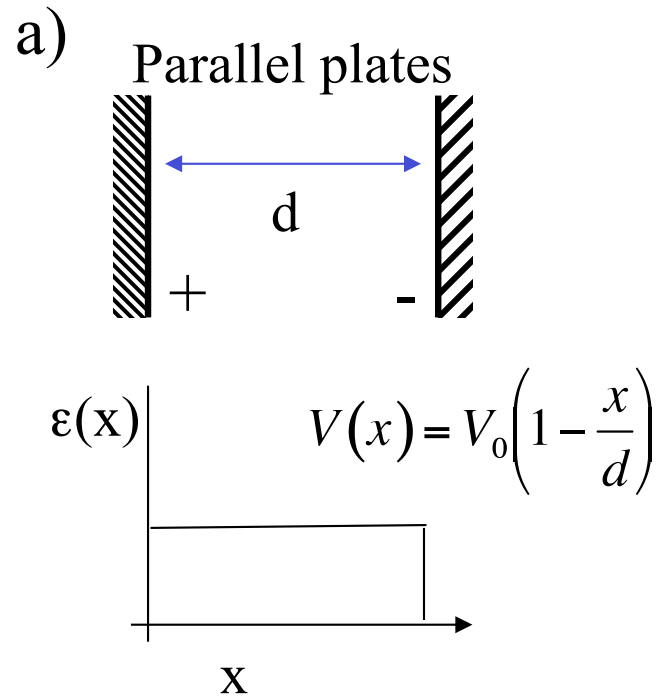

$$\epsilon(r) = \frac{V_0}{r \ln(b/a)}$$


Fig. 6.4

Knoll, 3rd Ed.

Typical Case: wire radius, $a = 80 \mu\text{m}$ @ 2 kV & chamber radius 2cm

Proportional Counters – Townsend Avalanche

Start with one electron, each generation follows in proportion to give a distribution governed by the mean-free-path (w/ binary collisions).

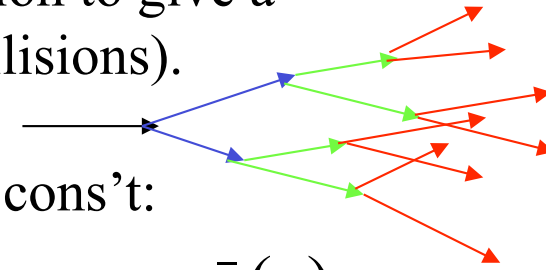

Uniform field produces exponential growth, $\alpha(E) = \alpha(r) = \text{const}$ 't:


$$\frac{dn^-}{dr} = +\alpha(r)n^- \rightarrow n^-(r) = n_0^- e^{\alpha r} \leftrightarrow M = \frac{n^-(r)}{n_0^-}$$

Non-uniform field requires a transformation $\alpha(E)$ to $\alpha(r)$ using dr/dE :

$$\int \frac{dn^-}{n^-} = \int \alpha(E) \frac{dr}{dE} dE$$

Townsend coefficients, α , depend on cross sections (mean free paths) and on “w” – thus depend on gas and are strong functions of E.

Additional mechanism of Penning ionization:
 $\text{Ne}^* + \text{Ar} \rightarrow \text{Ne} + \text{Ar}^+ + e^-$
 FIP (Ar) = 15.7 < E_1 (Ne) = 16.6
 FIP (Ne) = 21.5 eV

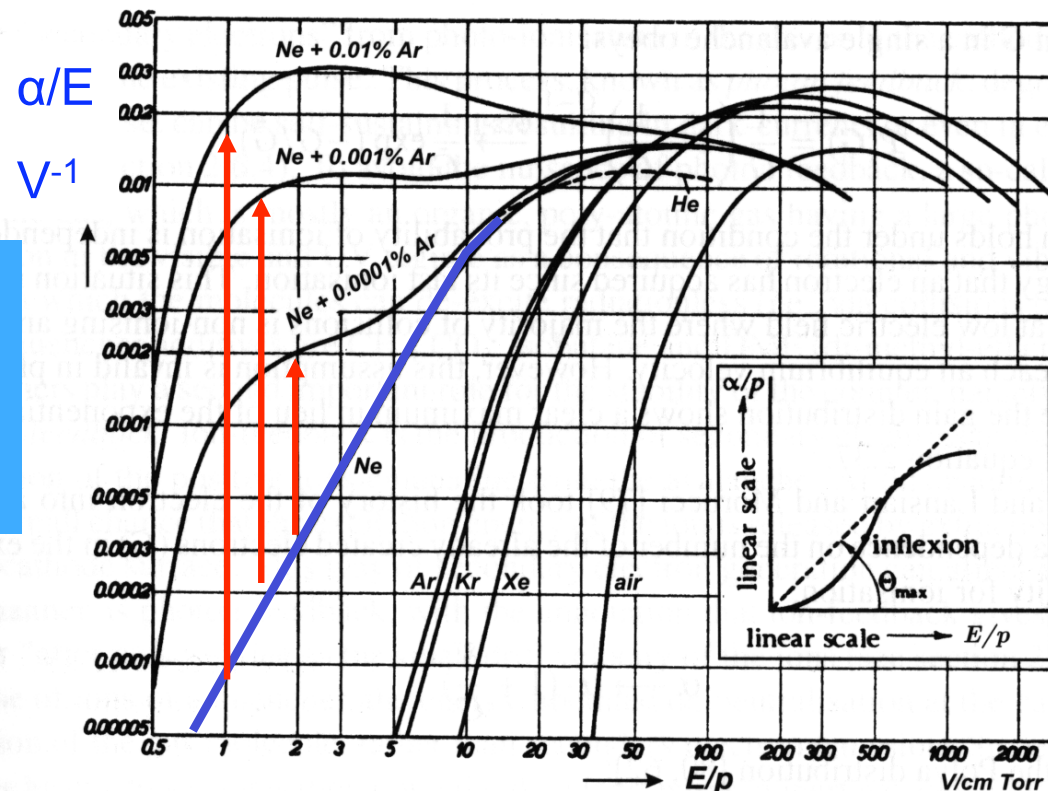

Proportional Counters – “M”

The general form for the multiplication factor, M, can be derived from simple arguments:

$$\int \frac{dn^-}{n^-} = \int \alpha(E) \frac{dr}{dE} dE$$

For a cylindrical detector:

$$E(r) \propto 1/r \quad \rightarrow \quad r \propto 1/E(r)$$

$$\ln M \propto \int_{r\text{-anode}}^{r\text{-crit}} \alpha(E) \left(\frac{1}{E^2} \right) dE$$

if $\alpha(E) \propto E$ [e.g. Ne+0.01Ar] then $\ln M \propto \ln E$

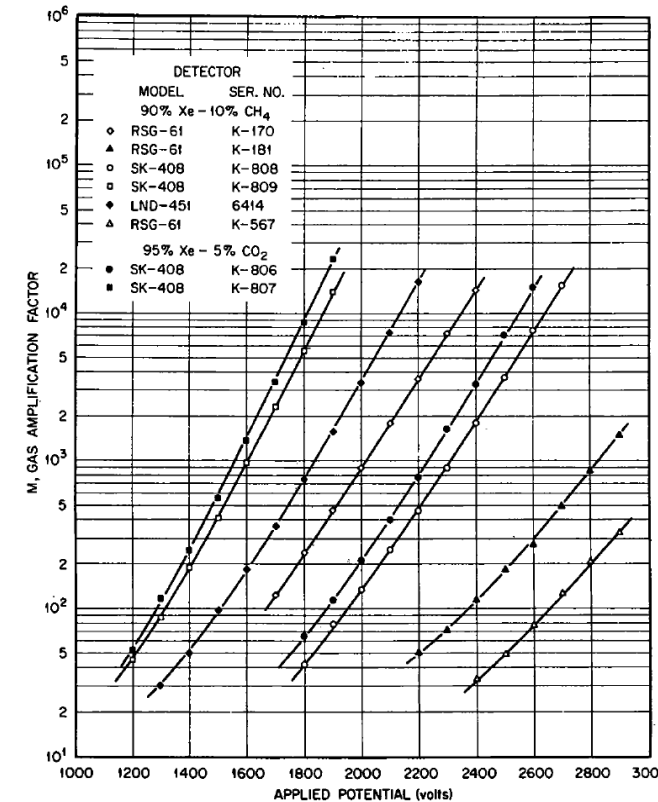


Fig. 6.10 Knoll, 3rd Ed.

$$\ln M = \frac{V}{\ln(b/a)} \frac{\ln 2}{\Delta V_\lambda} \left[\ln \left(\frac{V}{p a \ln(b/a)} \right) - \ln K \right] \quad \text{Eq. 6.8 in text}$$

Diethorn's equation with two parameters

that depend on the gas.

ΔV is the voltage drop in one MFP, K is the critical E/p for multiplication

Proportional Counters – Resolution

If the electrons don't have a history (reset at each mean-free path) then each ionization event is independent. The probability of such independent events follows the Flury Distribution of A with average \bar{A} :

$$P_{Flury}(A) = \frac{\left(1 - \frac{1}{\bar{A}}\right)^{A-1}}{\bar{A}} \rightarrow P_{Flury}(A) \approx e^{-\frac{A}{\bar{A}}} / \bar{A} \quad \sigma_A^2 = \bar{A}^2$$

The resolution of the total charge, Q, will have two contributions: variation of the primary charge production and the multiplication

$$Q = N_{IP} q_e M$$

$$\left(\frac{\sigma_Q}{Q}\right)^2 = \left(\frac{\sigma_N}{N_{IP}}\right)^2 + \left(\frac{\sigma_{qe}}{q_e}\right)^2 + \left(\frac{\sigma_M}{M}\right)^2 \quad \text{but } \sigma_N^2 = F N_{IP}$$

$$\left(\frac{\sigma_Q}{Q}\right)^2 = \left(\frac{F}{N_{IP}}\right) + \left(\frac{\sigma_M}{M}\right)^2$$


$$M = \bar{A} \equiv \frac{1}{N_{IP}} \sum_{i=1}^{N_{IP}} A_i = \frac{A_1}{N_{IP}} + \frac{A_2}{N_{IP}} + \dots \rightarrow \sigma_M^2 = \left[\left(\frac{\partial(A_i / N_{IP})}{\partial A} \right)^2 \sigma_{A_i}^2 + \dots \right]$$

$$\sigma_M^2 = \left(\frac{1}{N_{IP}} \right)^2 \sum_i \sigma_{A_i}^2 = \frac{1}{N_{IP}} \bar{\sigma}_A^2 \quad \text{but } \sigma_{A_1}^2 = \sigma_{A_2}^2 \dots = \bar{\sigma}_A^2$$

$$\left(\frac{\sigma_Q}{Q}\right)^2 = \left(\frac{F}{N_{IP}}\right) + \left(\frac{1}{N_{IP}}\right)$$

$$\frac{\sigma_M^2}{M^2} = \frac{1}{N_{IP}} \frac{\sigma_A^2}{M^2} \quad \text{but } M^2 = \bar{A}^2 = \sigma_A^2$$

The text argues that $(\sigma_A / A)^2$ is < 1 ... perhaps $1/2$.

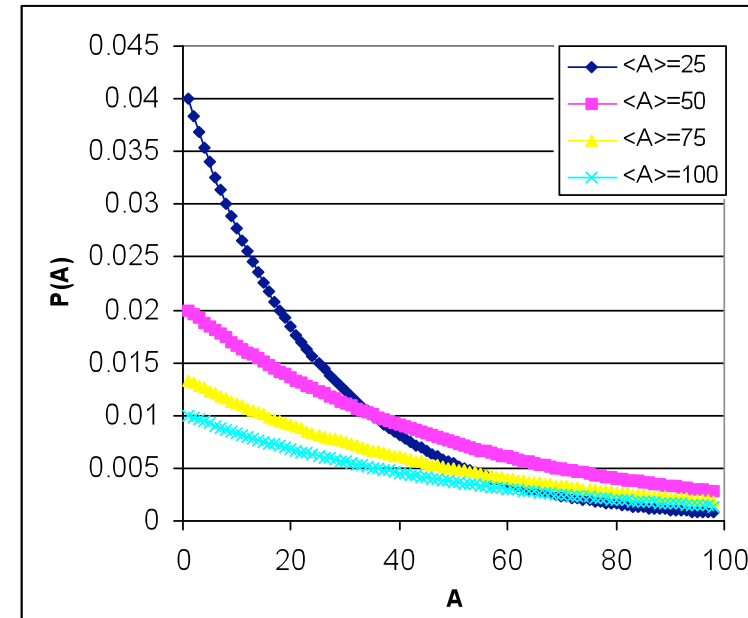

Proportional Counters – some difficulties


Approximately $\frac{1}{2}$ of the charge is created $\sim \lambda_{\text{MFP}}$ from the anode. The motion of the cations *away* from the anode induces the signal.

Fast rising signal; HV is shielded, slow cations have a long way to move to be neutralized on cathode. [use grids]


Multiplication process produces much more radiation damage to filling gas than primary ionization – no problem for noble gases (see below) but can damage anode itself.

Gas mixtures? The number of atoms in excited states will grow in proportion to the multiplication. The excited states tend to decay by photon emission rather than by Penning ionization – the photons are often UV and strike the cathode (wall). Being metal, the cathode will tend to emit a photoelectron ... similarly the collision of an atomic ion with the cathode during the neutralization can release an electron.

“Quench gas”: Mix in a small amount of a small molecule – molecules have vibrational modes that can absorb energy and they tend not to radiate UV photons (IR more likely). Also these molecules will tend to collect the charge due to charge-exchange reactions and are less likely to emit electrons from the cathode on neutralization. However, these molecules tend to get damaged – flow gas. Most used mixture: “P-10” 90% Ar 10% methane

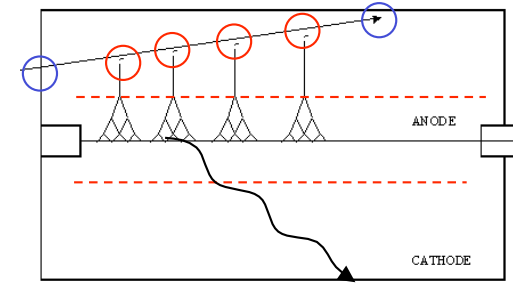


Beware of Cartoon !

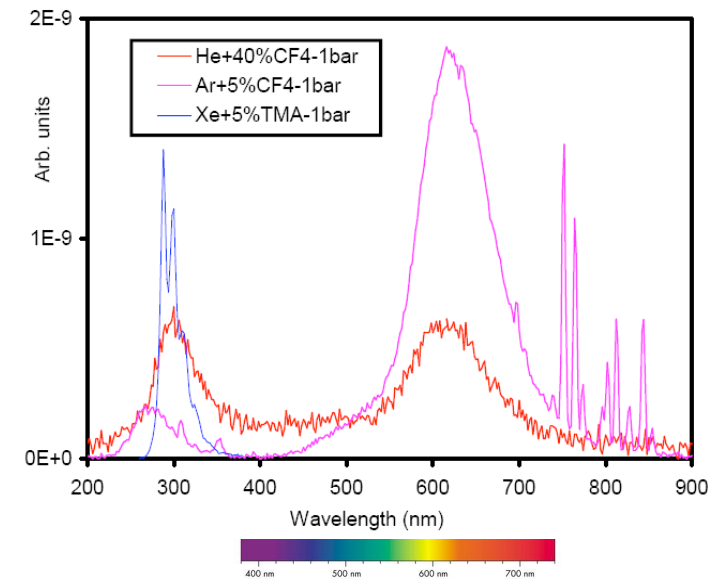


T.L. van Vuure, Ph.D, TU-Delft, 2004

Proportional Counters – Multiwires & Position

Field lines are approximately perpendicular to wire plane at large distances – electrons drift towards plane and retain position information. Many “wire chambers” have been developed to measure the positions of various particles.

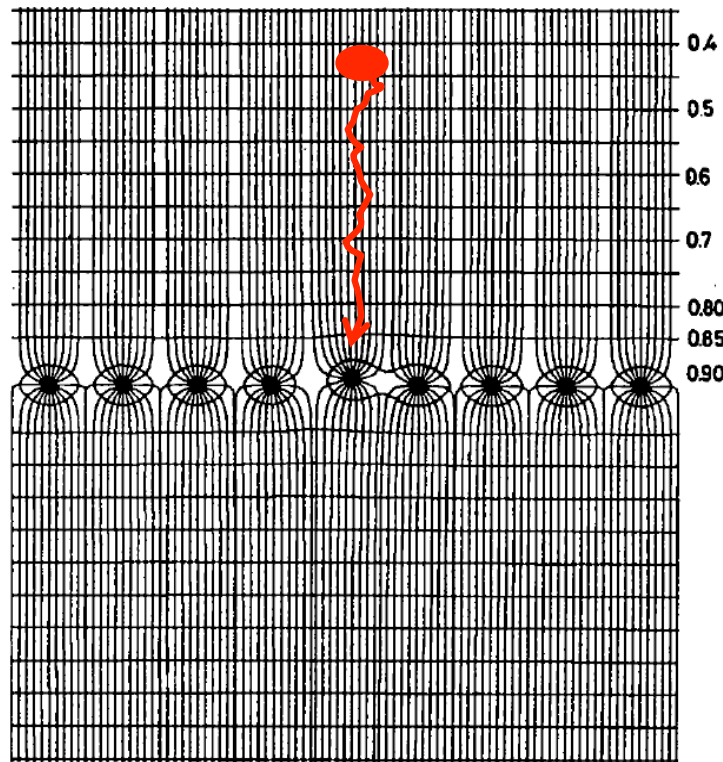

Figs. 6.19 & 20 Knoll, 3rd Ed.

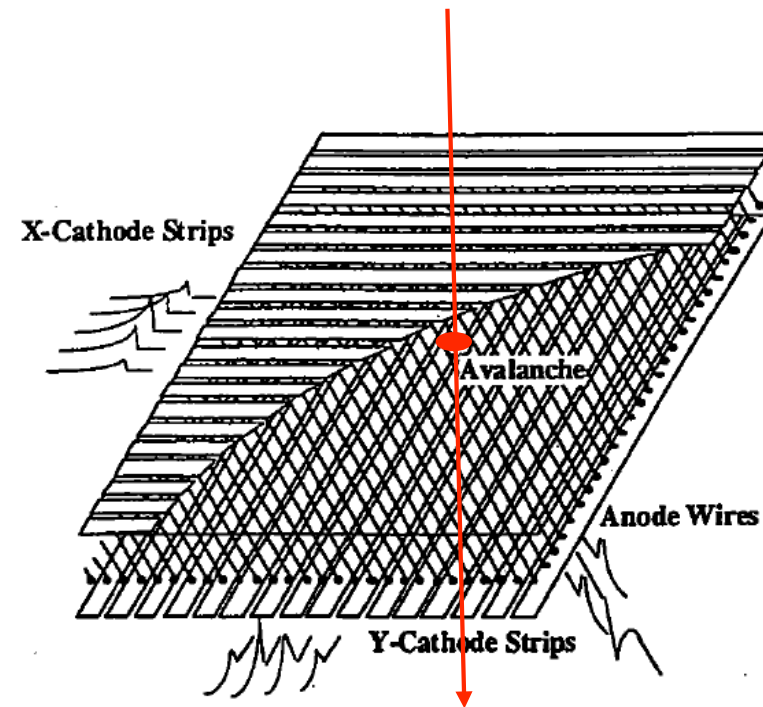


Read primary signal on wires, induced signals on cathode strips top and bottom – calculate 2D position.

Proportional Counters – Wires → Stripes


More sensitive detectors require more amplification – smaller “wires.”
Tiny anodes can be made by photoetching techniques but they must be supported on substrates (thick materials). Importantly the distance to the cathode traveled by the slow cations can be reduced enormously.

Multi-wire proportional chamber

Charpak

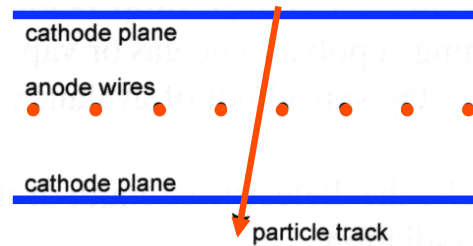


MWPC

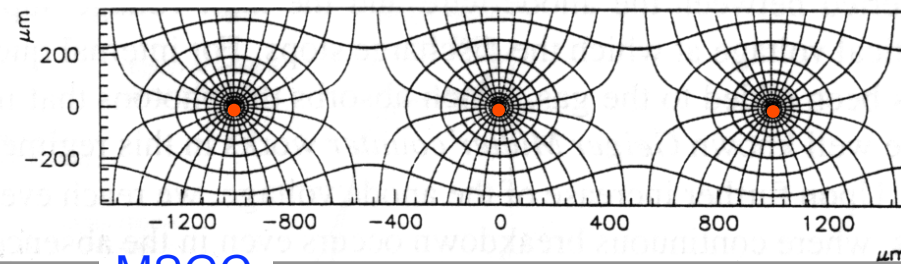


Micro-strip gas chamber

Oed

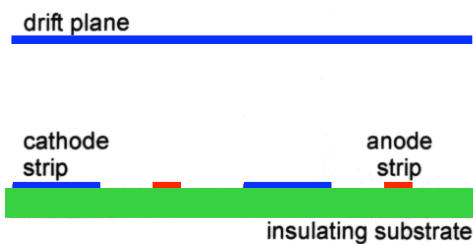


MSGC

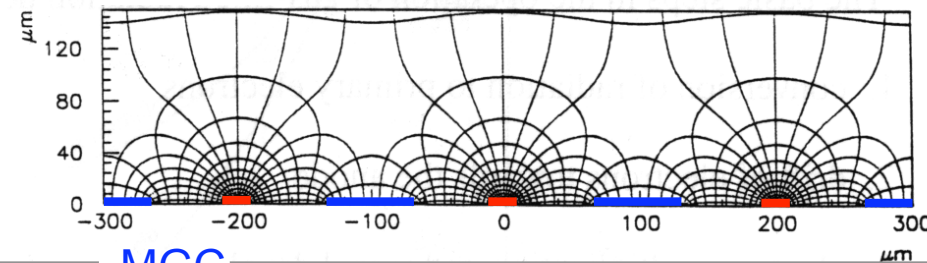


Micro-gap chamber

Bellazini

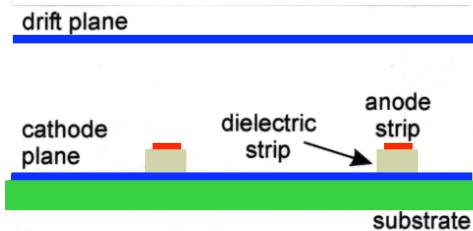


MGC

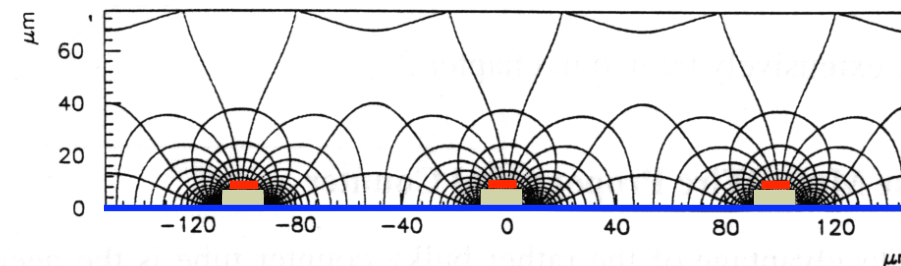


Proportional Counters – Wires → Stripes, Nope!

Thin metal strips on insulating support, generally resistive glass have a very high rate capability due to high fields and short distance of travel for the cations.




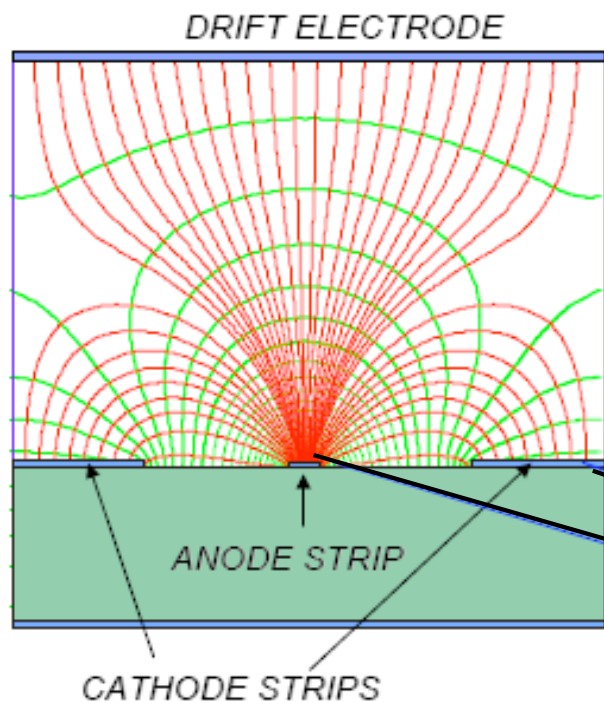


However, strips are permanently damaged by sparks or other discharges which kills the detector.

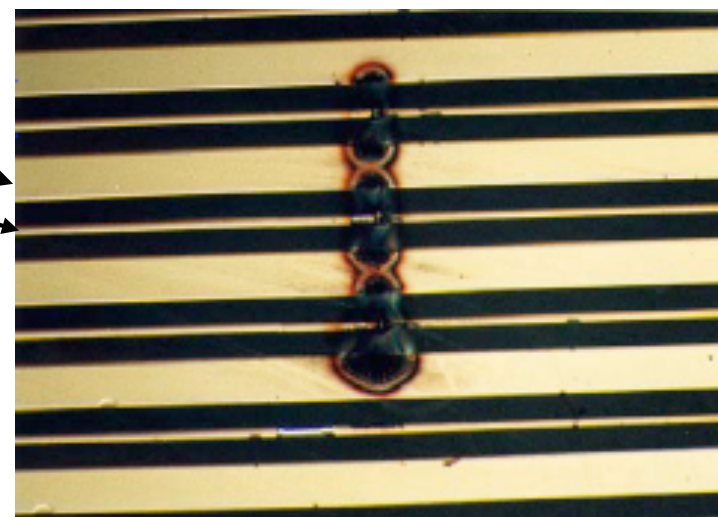

Proportional Counters – Micro Frisch Grid

MicroMeGas detectors are made on a tiny scale with micro fabrication techniques. These devices have high spatial resolution but may be gain limited because they are only one-stage by definition. Also they can be integrated with electronics, but they are generally small.

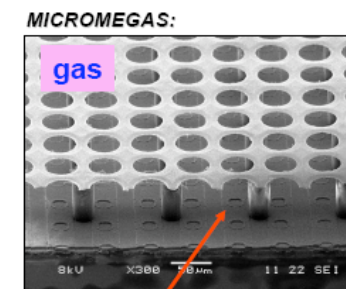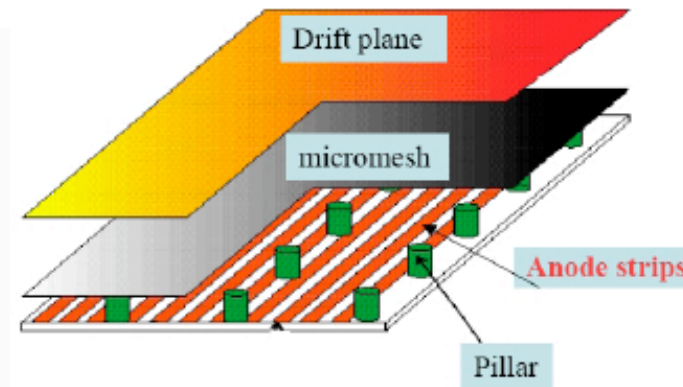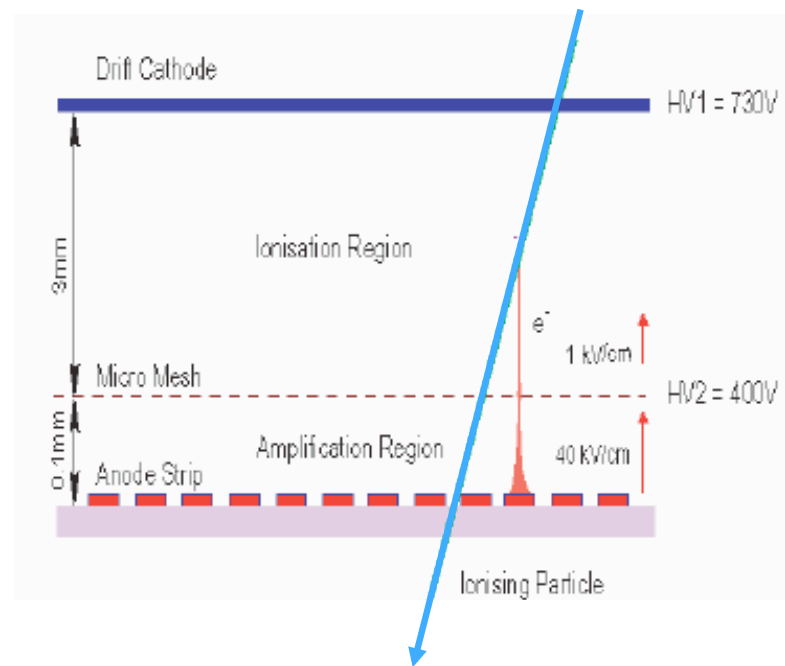

Y. Giomataris, et al. NIM A376 (1996) 239

14x14 mm² , 256x256 pixels, 55x55 µm²


H. Van der Graaf, IEEE-NSS workshop, 2007

Proportional Counters – Wires → Holes


Get rid of the wires and use holes in an insulator... Gas Electron Multiplier (GEM). Typically a plastic foil, Kapton 50 μm , metal plated on both sides with small holes $\sim 50 \mu\text{m}$ diameter. This creates a very high electric field 'in' the holes, perhaps 20kV/cm depending on the details. They can be stacked to get high gain.

Multi-wire proportional chamber

Charpak

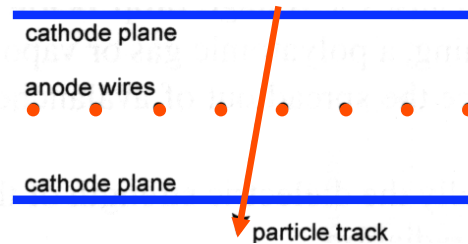


MWPC

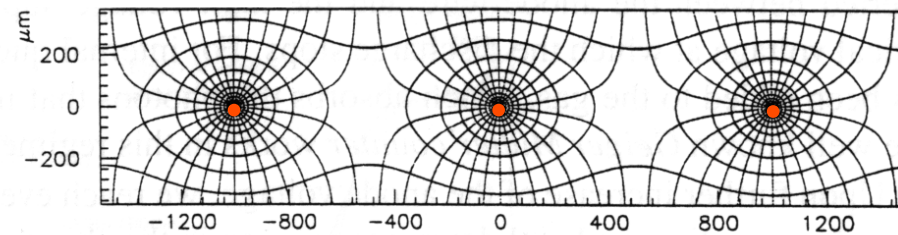


Gas Electron Multiplier

Sauli, NIM A433 (1997) 531

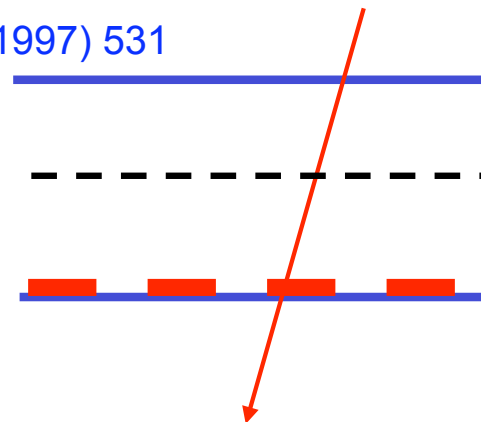


GEM

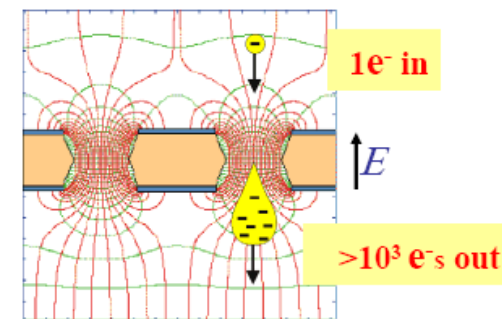

Electric field in the holes > 20kV/cm


Amos Breskin,
Thick GEM, 2008

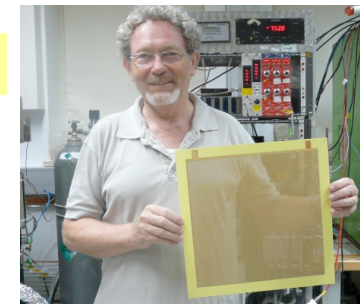

Proportional Counters – PPAC

Transmission detectors in the path of the beam should be highly uniform.
 Opinion: The MWPC devices are not suitable for radioactive ion beams ...
 parallel-plate avalanche counters



NSCL PPAC, NIM A 348 (1994)314

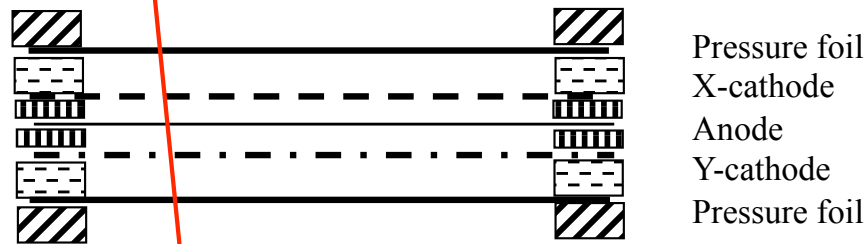

$V_0 \sim 500 \text{ V}$, $p = 5 \text{ torr}$,
 $\sim 3\text{mm}$ gap anode-cathode

$$\frac{\epsilon}{p} = \frac{500 \text{ V}}{0.003 \text{ m}} \frac{760 \text{ torr / atm}}{5 \text{ torr}} = 20 \frac{\text{MV}}{\text{m atm}}$$

Resistive charge division

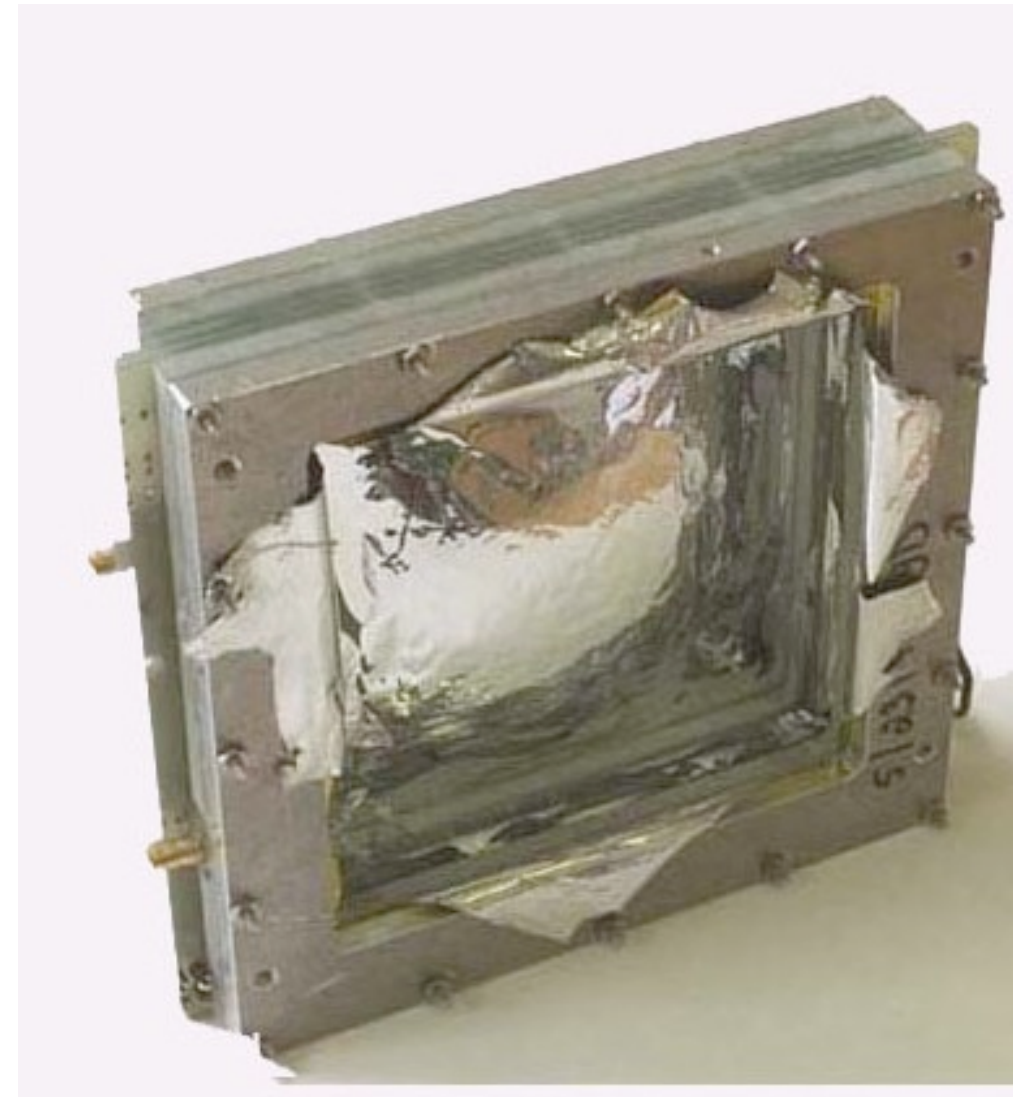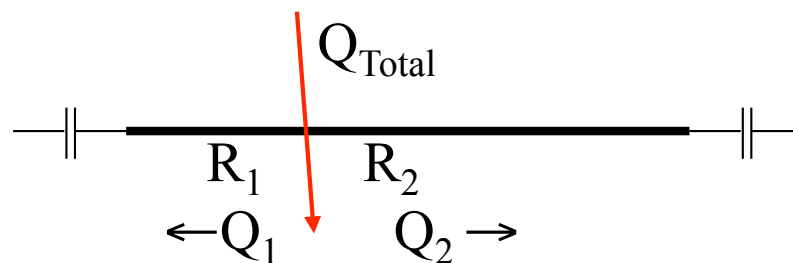


Chap. 7 Geiger-Mueller Counters


Increase field in Proportional counter so that the avalanche spreads along the entire length of the wire ... this will produce the largest signal but a sheath of cations will terminate the applied field.

Rutherford & Geiger, 1908

Recombination at the wall leads to “after pulse”





GM tubes are sealed ... “M” gets burned up.

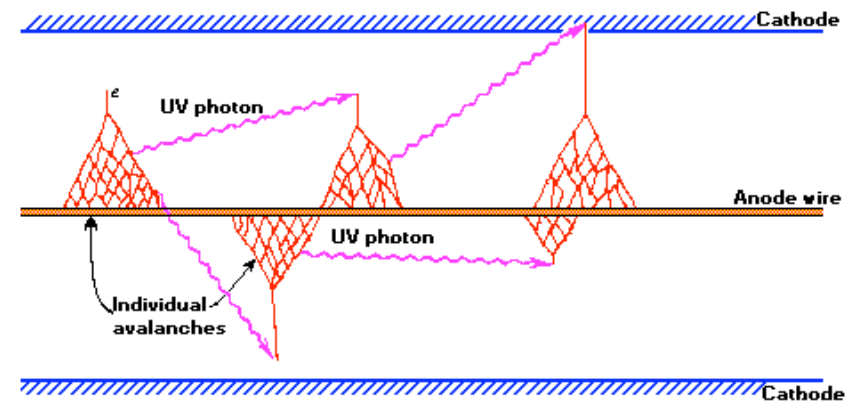

Beware of cartoon !

Hans Geiger (1882-1945) was a German physicist who introduced the first reliable detector for alpha particles and other ionizing radiation. His basic design is still used, although more advanced detectors also exist. His first particle counter was used in experiments that identified alpha particles as being the same as the nucleus of a Helium atom. He accepted his first teaching position in 1925 at the University of Kiel, where he worked with Walther Müller to improve the sensitivity and performance of his particle counter.

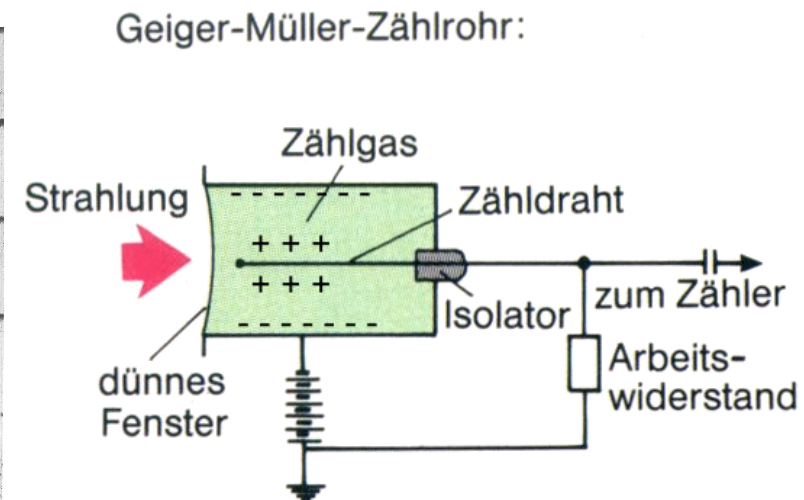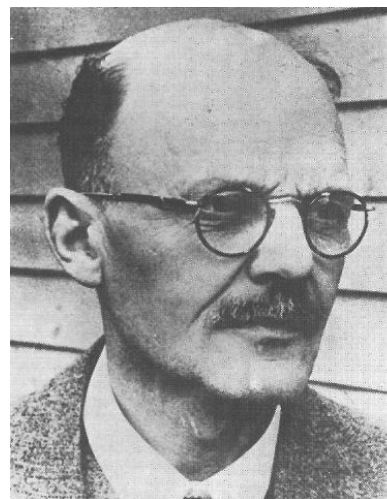

Geiger-Mueller Counter Example

Typical device: 1 atm P-10 gas (90%Ar, 10%CH₄)
Anode: $r_a \sim 30 \mu\text{m}$; Cathode $r_b \sim 1 \text{ cm}$; 10 cm long

$M \sim 10^6$ gives $V_R \sim 1 \text{ V}$ – Estimate V_0 , τ , C & R

